

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

Applicants: Tom FRANCKE and Christer ULLBERG
Application No.: NEW APPLICATION
Filed: December 4, 2003
For: COHERENT SCATTER IMAGING

PRIORITY LETTER

December 4, 2003

Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Dear Sirs:


Pursuant to the provisions of 35 U.S.C. 119, enclosed is/are a certified copy of the following priority document(s).

<u>Application No.</u>	<u>Date Filed</u>	<u>Country</u>
0302900-6	November 3, 2003	Sweden

In support of Applicant's priority claim, please enter this document into the file.

Respectfully submitted,

HARNESS, DICKY, & PIERCE, P.L.C.

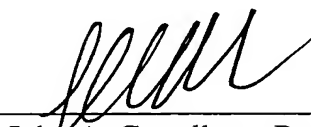By 
John A. Castellano, Reg. No. 35,094
P.O. Box 8910
Reston, Virginia 20195
(703) 668-8000

JAC/jj

PRV

PATENT- OCH REGISTRERINGSVERKET
Patentavdelningen

Intyg Certificate

Härmed intygas att bifogade kopior överensstämmer med de handlingar som ursprungligen ingivits till Patent- och registreringsverket i nedannämnda ansökan.

This is to certify that the annexed is a true copy of the documents as originally filed with the Patent- and Registration Office in connection with the following patent application.

(71) Sökande XCounter AB, Danderyd SE
Applicant (s)

(21) Patentansökningsnummer 0302900-6
Patent application number

(86) Ingivningsdatum 2003-11-03
Date of filing

Stockholm, 2003-11-13

För Patent- och registreringsverket
For the Patent- and Registration Office


Hjordis Segerlund

Avgift
Fee 170:-

46 8 6612119

Ink. t. Patent- och reg.verket

1

2003 -11- 0 3

COHERENT SCATTER IMAGING

Ink. t. Patent- och reg.verket

2003 -11- 0 3

FIELD OF THE INVENTION

The invention relates generally to apparatuses and methods for obtaining coherent scatter imaging data of an examination object.

BACKGROUND OF THE INVENTION AND RELATED ART

An X-ray medical diagnostic method such as mammography is a low-dose procedure that creates one or more images of a part of a patient such as a breast thereof, which is to be examined, e.g. for detection of early stages of cancer.

The mammography diagnostic procedure generally includes obtaining two images of each of the patient's breasts, one from above and one from the side. A physician or radiologist then reviews the images of the breast, i.e., mammograms, to identify any breast cancer.

While this procedure is one of the best methods of detecting early forms of breast cancer, it is still possible for the detection of breast cancer to be missed by a physician or radiologist reviewing the mammograms. For example, breast cancer may be missed by being obscured by radiographically dense, fibroglandular breast tissue.

Coherent scatter imaging has been studied in an effort to detect early forms of breast cancer, see e.g. Coherent Scatter Computed Tomography - A Novel Medical Imaging technique, J.-P. Schlomka, A. Harding, U. van Stevendaal, M. Grass, and G. Harding, Medical Imaging 2003: Physics of Medical Imaging, M.J. Yaffe and L.E. Antonuk, Editors, Proceedings of SPIE, Vol. 5030, 2003, p. 256.

46 8 6612119

Ink: t. Patent- och reg.verket

2003 -11- 0 3

2

Huvudfaxen Kassar

5 The method is derived from ART methods described in the literature and is based on a back-projection step using data from measurement of the angular spread distribution of photons as scattered from an illuminated slice within the object to be examined.

SUMMARY OF THE INVENTION

10 However, the method disclosed by J.-P. Schlomka et al. suffers from a limited spatial resolution. Each individual signal is collected along the complete length of the area of interaction between the incident radiation beam and the examination object, i.e. along the complete of the trajectory of the radiation photons of the radiation beam within the object. The experimental setup includes certainly a collimator made of thin tungsten lamellae placed in front of the detector, but these
15 lamellae are only there to provide for an image with low spatial resolution; a 2D detector was modeled by a single 1D vertical detector column based on GSO crystals and photomultipliers.

20 A main object of the invention is therefore to provide apparatuses and methods, respectively, for providing coherent scatter imaging data with a better spatial resolution than what is obtainable by using the above-identified prior art method.

25 In this respect there is a particular object to provide such apparatuses and methods, which provide coherent scatter imaging data, by which high-quality one-, two-, and even three-dimensional images with high spatial resolution, scattering angular resolution, signal-to-noise ratio, dynamic range, and image contrast can be produced.

A still further object of the invention is to provide such apparatuses and methods, which provide conventional transmission

46 8 6612119

Ink. t. Patent- och reg.verket

2003 -11- 0 3

3

Huvudfaxen Kasse

imaging data simultaneously with the coherent scatter imaging data.

5 A yet further object of the invention is to provide such apparatuses and methods, which are reliable, accurate, uncomplicated and inexpensive.

These objects, among others, are attained by apparatuses and methods as claimed in the appended claims.

10 In order for the invention to operate properly, unwanted scattered radiation has to be discriminated from being detected to a particularly large extent. The line detectors, on which the present invention are based, have each an elongated opening for entry of a respective fan-shaped coherently scattered ray bundle; a row of individual elongated detector elements arranged essentially parallel with the
15 elongated opening; and is of the kind wherein charges or photons generated by interactions between the respective fan-shaped coherently scattered ray bundle and a detection medium within the line detector and traveling in a direction essentially perpendicular to the respective fan-shaped coherently scattered
20 ray bundle, are detected by the row of individual detector elements. Such edge-on detectors can be made extremely direction sensitive.

25 Further characteristics of the invention, and advantages thereof, will be evident from the detailed description of preferred embodiments of the present invention given hereinafter and the accompanying Figs. 1-3, which are given by way of illustration only, and thus are not limitative of the present invention.

46 8 6612119

Ink. t. Patent- och reg.verket

2003 -11- 0 3

Huvudfaxen Kåsson

4

BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 illustrates schematically, in a side view, an apparatus for obtaining coherent scatter imaging data for x-ray examination of an object according to a preferred embodiment of the present invention.

Fig. 2a illustrates schematically, in a cross-sectional side view, a line detector comprised in the apparatus of Fig. 1.

Fig. 2b illustrates schematically a cross-sectional view of the detector of Fig. 2a along the line I-I.

Fig. 3a illustrates schematically, in a side view, an apparatus for obtaining coherent scatter imaging data for x-ray examination of an object according to a further preferred embodiment of the present invention.

Fig. 3b illustrates schematically, in a perspective view, portions of the apparatus of Fig. 3b.

Identical reference numerals are used throughout the Figures to denote identical or similar components, portions, details and the like of the various embodiments.

DESCRIPTION OF PREFERRED EMBODIMENTS

The apparatus of Fig. 1 comprises a divergent X-ray source 1, which produces X-rays 2 centered around an axis of symmetry 3; an aperture collimator 4 having a circular opening for collimating the emitted X-rays 2 to form a well defined collimated radiation beam 2a; a radiation detector arrangement 6; and a device 7 for rigidly connecting the X-ray source 1, the collimator 4, and the radiation detector arrangement 6 to each other and moving the X-ray source 1, the collimator 4, and the radiation detector arrangement 6 relative an object 5,

46 8 6612119.

Ink. t. Patent- och reg.verket

7003 -11- 0 3

5

Huvudfaxen Kassen

which is to be examined, to scan the object 5. Alternatively, the X-ray source 1, the collimator 4, and the radiation detector arrangement 6 are held still and the object 5 is moved during the scanning.

- 5 The radiation detector arrangement 6 comprises a stack of line detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_N$ directed towards different positions of the trajectory 2b of the radiation beam 2a in the examination object 5 to allow different fan-shaped ray bundles $b_1, \dots, b_{n-1}, b_{n+1}, \dots, b_N$ of the radiation beam 2a as coherently
- 10 scattered in different small portions of the examination object 5 along the trajectory 2b to enter the line detectors and be detected therein. The line detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_N$ are preferably directed towards the different positions along the trajectory 2b of the radiation beam 2a in the object 5,
- 15 which directions define angles $\alpha_1, \dots, \alpha_{n-1}, \alpha_{n+1}, \dots, \alpha_N$ with respect to the axis of symmetry 3 in the xz-plane, in which the axis of symmetry 3 and the stack of line detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_N$ subsist, which angles $\alpha_1, \dots, \alpha_{n-1}, \alpha_{n+1}, \dots, \alpha_N$ have the same magnitude.
- 20 One of the line detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_N$ is illustrated more in detail in Figs. 2a-b. The line detector has an elongated opening 30 for entry of the fan-shaped coherently scattered ray bundle; a row of elongated individual detector elements or strips 27 arranged essentially parallel with the
- 25 elongated opening 30; and is of the kind wherein charges or photons generated by interactions between the fan-shaped coherently scattered ray bundle entered into the detector and a detection medium 24 within the line detector and traveling in a direction essentially perpendicular to the fan-shaped
- 30 coherently scattered ray bundle, can be detected by the row of individual detector elements 27.

46 8 6612119

Ink. t. Patent- och reg.verket

2003 -11- 0 3

6

Huvudfaxen Kassen

Preferably, the line detector is a gaseous-based parallel plate detector, especially a detector wherein avalanche amplification is performed to amplify the signals, comprising substantial planar cathode 25, 26 and combined anode/readout 27, 28 arrangements. Each of the electrode arrangements 25, 26; 27, 28 includes an electrically conducting electrode layer 25, 27 supported by a respective dielectric substrate 26, 28, wherein the arrangements are oriented so that the conductive cathode 25 and anode 27 layers are facing each other.

Preferably, the dielectric substrates 26, 28 and the window 30 define together with sidewalls 29, 31, 32 a gas-tight confinement capable of being filled with an ionizable gas or gas mixture. Alternatively, the electrode arrangements are arranged within an external gas-tight casing (not illustrated). The ionizable gas or gas mixture may e.g. comprise krypton and carbon dioxide or xenon and carbon dioxide.

Such gaseous-based parallel plate detector has been found to be capable to be made extremely direction sensitive, and thus very suitable for use in applications where unwanted scattered radiation has to be strongly attenuated. In fact the view of field of the gaseous-based parallel plate detector, schematically indicated by b in Fig. 2a, is extremely thin - much thinner than the width of the window 30 and thinner than a typical thickness of the fan-shaped coherently scattered ray bundle entered into the detector. The discovery of this property was an absolute prerequisite for inventing an apparatus for high-energy radiographic measurement of an object, which prevents Compton scattered radiation from being detected, see our pending U.S. Patent Application No. xxxx [numret för spridningsfri detection ska in här], the contents of which being incorporated by reference. Similarly, the property

46 8 6612119

Ink. t. Patent- och reg.verket

7

2003 -11- 0 3

Huvudfaxen Kassar

is very important for the present invention - in order to obtain sufficient spatial resolution.

For further details regarding different kind of detectors for use in the present invention, reference is made to the following

5 U.S. Patents by Tom Francke et al. and assigned to XCounter AB of Sweden, which patents are hereby incorporated by reference: Nos. 6,118,125; 6,373,065; 6,337,482; 6,385,282; 6,414,317; 6,476,397; 6,477,223; 6,518,578; 6,522,722; 6,546,070; 6,556,650; 6,600,804; and 6,627,897.

10 Alternative detectors to be used in the present invention include other kinds of direction sensitive detectors, e.g. silicon PIN-diodes with edge-on incidence of radiation.

The individual conductive anode/readout elements 27 are arranged side by side in a row orthogonal to the xz-plane and

15 define a respective angle β_1, \dots, β_M with respect to the xz-plane so that all the anode/readout elements 27 point towards a single point of the interaction trajectory 2b of the radiation beam 2a with the object 5, and detect therefore different angular portions β_1, \dots, β_M of the fan-shaped ray

20 bundle entered into the line detector.

The line detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_N$ are thus capable to simultaneously record coherent scatter imaging data sufficient to form a plurality of one-dimensional images, each being composed of radiation as coherently scattered in the

25 examination object 5 in a respective angle β_1, \dots, β_M - one signal from each of the line detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_N$ is needed to form each of the plurality of one-dimensional images.

The radiation detector arrangement 6 of the apparatus of Fig. 1 comprises also a detector $6a_n$ arranged in the path of the

30

46 8 6612119

Ink. t. Patent- och reg.verket

2003 -11- 0 3

8

Huvudfaxen Kasse

radiation beam 2a to measure the transmission through the examination object 5 simultaneously with the simultaneous recording of the coherent scatter imaging data. The detector 6a_n may be a point detector or may be a detector of the kind as described with reference to Figs. 2a-b to not only measure the transmission by an anode/readout element arranged with a β -angle (i.e. an angle with respect to the xz-plane) of 0°, but also radiation photons coherently scattered in the yz-plane.

Still further, the device 7 is provided for moving the radiation source 1, the collimator 4, and the radiation detector arrangement 6 relative the object 5 in a direction in the xy-plane (i.e. in a plane orthogonal to the axis of symmetry 3), while the individual line detectors 6a₁-6a_{n-1}, 6a_{n+1}-6a_N together record a plurality of line images of radiation as coherently scattered in the object 5 in the angles β_1, \dots, β_M to thereby produce coherent scatter imaging data sufficient to form a plurality of two-dimensional images, each being composed of radiation as coherently scattered in the object 5 in a respective one of the angles β_1, \dots, β_M . A line image of the radiation as transmitted through the object is obtained concurrently by the detector 6a_n.

The device 7 may additionally be adapted to move the divergent radiation source 1 and the radiation detector arrangement 6 relative the object 5 in second direction in the xy-plane, while the line detectors 6a₁-6a_{n-1}, 6a_{n+1}-6a_N together record a plurality of line images of radiation as scattered in the object 5 in the angles β_1, \dots, β_M to thereby produce coherent scatter imaging data sufficient to form a plurality of three-dimensional images, each being composed of radiation as coherently scattered in the object 5 in a respective one of the angles β_1, \dots, β_M . A two-dimensional image of the radiation

2003 -11- 0 3

Huvudfoxen Kassar

as transmitted through the object is obtained concurrently by the detector $6a_n$.

Turning now to Figs. 3a-b, a second preferred embodiment of the present invention will be described. The collimator 4 comprises here a slit shaped opening, where the slit extends in the y-direction and as a consequence, the radiation beam 2a is substantially sheet-shaped. The openings of the line detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_n$ are parallel with the substantially sheet-shaped radiation beam 2a, and the line detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_n$ are directed towards the same small portion of the trajectory 2b of the radiation beam 2a in the examination object 5, and the detector elements 27 of each of the line detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_n$ are separated, elongated and arranged to provide coherent scatter imaging data sufficient to form one of a plurality of one-dimensional images.

However, actions have to be taken to reduce scattered radiation in the plane of the detector, otherwise the images will be blurred. One solution is to arrange the detector arrangement 6 very far from the object 5. Alternatively, or additionally, the detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_n$ may be made very long in the direction of the incident radiation to be detected, the anode/readout elements 27 may be arranged in the far end only of the detectors, the detectors may be provided with anti-scatter grids in their front ends, and/or radiation absorbing interstitial barriers may be provided in between each of the anode/readout elements 27 to prevent unwanted scattered radiation in the plane of the detector from crossing several of the anode/readout elements 27, and to consequently blur the image recorded.

46 8 6612119

Svenskt Patent- och reg.verket

2003 -11- 0 3

10

Huvudfaxen Kassar

The line detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_N$ define different angles $\alpha_1-\alpha_{n-1}$, $\alpha_{n+1}-\alpha_N$ with respect to the axis of symmetry 3 in the xz-plane (i.e. the plane in which the axis of symmetry 3 and the stack of line detectors subsist).

5 The radiation detector arrangement 6 may like in previous embodiment comprise a detector $6a_n$ arranged in the path of the radiation beam 2a to measure the transmission through the examination object 5 simultaneously with the simultaneous recording of the coherent scatter imaging data. Preferably,
10 the detector $6a_n$ is a line detector similar to the other line detectors described in this description, which line detector $6a_n$ performs instantaneous one-dimensional imaging of the cross section of the substantially sheet-shaped radiation beam 2a.

The apparatus of Fig. 3a may further comprise the device 7 for
15 moving the radiation detector arrangement 6 and optionally the radiation source 1 relative the object 5, while the line detectors $6a_1-6a_{n-1}$, $6a_{n+1}-6a_N$ together record a plurality of line images of radiation as scattered in the object 5 in a plurality of different angles $\alpha_1-\alpha_{n-1}$, $\alpha_{n+1}-\alpha_N$ to thereby produce
20 coherent scatter imaging data sufficient to form a plurality of images, each being composed of radiation as coherently scattered in the examination object in a respective angle $\alpha_1-\alpha_{n-1}$, $\alpha_{n+1}-\alpha_N$. The device may move the radiation source 1 and the radiation detector arrangement 6 relative the object 5 in any
25 direction in the xz-plane. If scanning is performed in two different directions three-dimensional coherent scatter imaging data can be produced. A two- or even three-dimensional image of the radiation as transmitted through the object is obtained concurrently by the detector $6a_n$.

30 In summary, by the Figs. 1-2 embodiment one-dimensional images of coherently scattered radiation in the examination object is

46 8 6612119

Ink. t. Patent- och reg.verket..

2003 -11- 0 3

11

Huvudfaxen Kassen

obtained instantaneously in the z-direction. The number of pixels in each one-dimensional image is N-1, the number of images is M, and they are produced from radiation scattered off the radiation beam both in the yz- and xz-planes.

- 5 Simultaneous point measurement of transmission is obtained. Scanning is performed in the xy-plane. By the Fig. 3 embodiment one-dimensional images of coherently scattered radiation in the examination object is obtained instantaneously in the y-direction. The number of pixels in
- 10 each one-dimensional image is M, the number of images is N-1, and they are produced from radiation scattered off the radiation beam in the xz-plane. Simultaneous one-dimensional measurement of transmission is obtained. Scanning is performed in the xz-plane.

15



46 8 6612112

Int. Patent- och reg.verket

2003 -11- 0 3

12

Huvudfaxen Kassar

CLAIMS

1. An apparatus for obtaining coherent scatter imaging data of an examination object (5), characterized in:

- 5 - a radiation source arrangement (1, 4) for creating a radiation beam (2a) of ionizing radiation centered around an axis of symmetry (3), which radiation beam (2a) is directed through said examination object (5); and
- 10 - a radiation detector arrangement (6) comprising a stack of line detector units ($6a_1-6a_{n-1}, 6a_{n+1}-6a_n$), each being directed towards a small portion of the trajectory (2b) of said radiation beam (2a) in said examination object (5) to allow a substantially fan-shaped ray bundle ($b_1-b_{n-1}, b_{n+1}-b_n$) of said radiation beam (2a) as coherently scattered in said examination object to enter the line detector unit and be
- 15 detected therein; wherein
- each of said line detector units has an elongated opening (30) for entry of the respective fan-shaped coherently scattered ray bundle; a row of individual detector elements (27) arranged essentially parallel with said elongated
- 20 opening; and is of the kind wherein charges or photons generated by interactions between the respective fan-shaped coherently scattered ray bundle and a detection medium within the line detector unit and traveling in a direction essentially perpendicular to the respective fan-shaped
- 25 coherently scattered ray bundle, are detected by said row of individual detector elements; and
- said line detector units and their respective individual detector elements are formed and oriented so as to allow simultaneous recording of coherent scatter imaging data
- 30 sufficient to form a plurality of one-dimensional images, each

46 8 6612119

Ink. t. Patent- och reg.verket

2003 -11- 0 3

13

Huvudfaxen Kassan

being composed of radiation as coherently scattered in said examination object in a respective angle ($\beta_1 - \beta_M$; $\alpha_1 - \alpha_{n-1}$, $\alpha_{n+1} - \alpha_N$).

5 2. The apparatus of claim 1 wherein said line detector units are directed towards different positions along the trajectory (2b) of said radiation beam (2a) in said examination object (5) to allow different fan-shaped ray bundles of said radiation beam as coherently scattered in different small portions of said examination object to enter said line
10 detector units and be detected therein so that a signal from each of said line detector units is needed to form one of said plurality of one-dimensional images.

3. The apparatus of claim 2 wherein

15 - the row of detector elements of each of said line detector units is essentially orthogonal to a plane (xz), in which said axis of symmetry (3) and said stack of line detector units subsist; and

20 - the detector elements of each of said line detector units are separated, elongated and directed so their extension lines converge in a single point in said small portion, and detect therefore different angular portions of the fan-shaped ray bundle entered into the respective line detector unit so that a signal from each of said line detector unit is needed to form each of said plurality of one-dimensional images.

25 4. The apparatus of claim 2 or 3 wherein said line detector units are directed towards different positions along the trajectory (2b) of said radiation beam (2a) in said examination object (5), which directions define angles ($\alpha_1 - \alpha_{n-1}$, $\alpha_{n+1} - \alpha_N$) with respect to said axis of symmetry (3) in the plane

2003 -11- 0 3

14

Huvudfaxen Kassen

(xz), in which said axis of symmetry and said stack of line detector units subsist, which angles have the same magnitude.

5 5. The apparatus of any of claims 2-4 wherein said radiation detector arrangement (6) comprises a detector unit ($6a_n$) arranged in the path of said radiation beam (2a) to measure the transmission through said examination object (5) simultaneously with said simultaneous recording of coherent scatter imaging data.

10 6. The apparatus of any of claims 2-5 wherein each of said line detector units is a gaseous-based parallel plate (25-28) detector.

7. The apparatus of claim 6 wherein each of said line detector units is an avalanche amplification detector.

15 8. The apparatus of any of claims 2-7 further comprising a device (7) for moving said radiation source and said radiation detector arrangement relative said examination object in a direction in a plane orthogonal (xy) to said axis of symmetry (3), while said line detector units are together adapted to record a plurality of line images of radiation as scattered in
20 said examination object in a plurality of different angles (β_1 - β_M) to thereby produce coherent scatter imaging data sufficient to form a plurality of two-dimensional images, each being composed of radiation as coherently scattered in said examination object in a respective angle.

25 9. The apparatus of any of claims 2-7 further comprising a device (7) for moving said radiation source and said radiation detector arrangement relative said examination object in two different directions in a plane (xy) orthogonal to said axis of symmetry (3), while said line detector units are together
30 adapted to record a plurality of line images of radiation as

2003 -11- 0 3

15

Huvudfoxen Kossan

5 scattered in said examination object in a plurality of different angles (β_1 - β_M) to thereby produce coherent scatter imaging data sufficient to form a plurality of three-dimensional images, each being composed of radiation as coherently scattered in said examination object in a respective angle.

10. The apparatus of claim 1 wherein

- said radiation beam (2a) of ionizing radiation has a substantially line-shaped cross-section;
- 10 - the openings of said line detector units are parallel with the substantially line-shaped cross-section of said radiation beam;
- said line detector units are directed towards the same small portion of the trajectory (2b) of said radiation beam in said examination object (5); and
- 15 - the detector elements of each of said line detector units are separated, elongated and arranged to provide coherent scatter imaging data sufficient to form one of said plurality of one-dimensional images.

20 11. The apparatus of claim 10 wherein said line detector units are directed towards the same small portion of the trajectory (2b) of said radiation beam (2a) in said examination object (5); which directions define different angles with respect to said axis of symmetry (3) in a plane (xz), in which said axis of symmetry and said stack of line detector units subsist.

25

12. The apparatus of claim 10 or 11 wherein said radiation detector arrangement (6) comprises a detector unit (6a_n) arranged in the path of said radiation beam (2a) to measure the transmission through said examination object (5)

46 8 6612119

Int. t. Patent- och reg.verket

2003 -11- 0 3

16

Huvudfaxen Kassan

simultaneously with said simultaneous recording of coherent scatter imaging data.

13. The apparatus of any of claims 10-12 wherein each of said line detector units is a gaseous-based parallel plate (25-28) detector, particularly a gaseous-based avalanche amplification parallel plate (25-28) detector.

14. The apparatus of any of claims 10-13 further comprising a device (7) for moving said radiation detector arrangement and optionally said radiation source relative said examination object, while said line detector units are together adapted to record a plurality of line images of radiation as scattered in said examination object in a plurality of different angles to thereby produce coherent scatter imaging data sufficient to form a plurality of images, each being composed of radiation as coherently scattered in said examination object in a respective angle.

15. A method for obtaining coherent scatter imaging data of an examination object (5), characterized by the steps of:

20 - directing a radiation beam (2a) of ionizing radiation centered around an axis of symmetry (3) through said examination object (5); and

25 - directing each one of a plurality of line detector units ($6a_1-6a_{n-1}$, $6a_{n+1}-6a_N$) arranged in a stack towards a small portion of the trajectory (2b) of said radiation beam in said examination object (5) to allow a substantially fan-shaped ray bundle (b_1-b_{n-1} , $b_{n+1}-b_N$) of said radiation beam as coherently scattered in said examination object to enter the line detector unit; and

- detecting said fan-shaped ray bundle entering into said line detector units, wherein

- each of said line detector units has an elongated opening (30) for entry of the respective fan-shaped coherently scattered ray bundle; a row of individual detector elements (27) arranged essentially parallel with said elongated opening; and is of the kind wherein charges or photons generated by interactions between the respective fan-shaped coherently scattered ray bundle and a detection medium within the line detector unit and traveling in a direction essentially perpendicular to the respective fan-shaped coherently scattered ray bundle, are detected by said row of individual detector elements; and

- said line detector units and their respective individual detector elements are formed and oriented so as to allow simultaneous recording of coherent scatter imaging data sufficient to form a plurality of one-dimensional images, each being composed of radiation as coherently scattered in said examination object in a respective angle.

16. The method of claim 15 wherein

- said line detector units are directed towards different positions along the trajectory (2b) of said radiation beam (2a) in said examination object (5) to allow different fan-shaped ray bundles of said radiation beam as coherently scattered in different small portions of said examination object to enter said line detector units and be detected therein;

- the row of detector elements (27) of each of said line detector units is essentially orthogonal to a plane (xz), in

46 8 6612119.

Ink. t. Patent- och reg.verket

2003 -11- 0.3

18

Huvudfaxen Kasse

which said axis of symmetry (3) and said stack of line detector units subsist; and

- the detector elements of each of said line detector units are separated, elongated and directed so their extension lines converge in a single point in said small portion, and detect therefore different angular portions of the fan-shaped ray bundle entered into the respective line detector unit so that a signal from each of said line detector unit is needed to form each of said plurality of one-dimensional images.

17. An apparatus for obtaining coherent scatter imaging data of an examination object (5), characterized in:

- a radiation source arrangement (1, 4) for creating a collimated radiation beam (2a) of ionizing radiation centered around an axis of symmetry (3), which radiation beam (2a) is directed through said examination object (5); and

- a line detector unit (6a₁) being directed towards a small portion of the trajectory (2b) of said radiation beam (2a) in said examination object (5) to allow a substantially fan-shaped ray bundle (b₁) of said radiation beam (2a) as coherently scattered in said examination object to enter the line detector unit and be detected therein; wherein

- said line detector unit has an elongated opening (30) for entry of the fan-shaped coherently scattered ray bundle; a row of individual detector elements (27) arranged essentially parallel with said elongated opening; and is of the kind wherein charges or photons generated by interactions between the fan-shaped coherently scattered ray bundle and a detection medium within the line detector unit and traveling in a direction essentially perpendicular to the fan-shaped

46 8 6612119.

Ink. t. Patent- och reg.verket

7003 -11- 0 3

19

Huvudfaxen Kassa

coherently scattered ray bundle, are detected by said row of individual detector elements;

- the row of detector elements of each of said line detector units is essentially orthogonal to said axis of symmetry (3);

5

and

- the detector elements of said line detector unit are separated, elongated and directed so their extension lines converge in a single point in said small portion, and detect therefore different angular portions of the fan-shaped ray bundle entered into the line detector unit.

10

0
1
2
3
4
5
6
7
8
9
A
B
C
D
E
F
G
H
I
J
K
L
M
N
O
P
Q
R
S
T
U
V
W
X
Y
Z
[
,
-
.
/

46 8 6612119.

Ink. t. Patent- och reg.verket

20

2003 -11- 0 3

Huvudfaxen Kassar

ABSTRACT

An apparatus for obtaining coherent scatter imaging data of an object (5) comprises a stack of line detectors ($6a_1-6a_{n-1}, 6a_{n+1}-6a_N$), each being directed towards a small portion of the trajectory (2b) of a radiation beam (2a) passed through the object (5) to allow a ray bundle ($b_1-b_{n-1}, b_{n+1}-b_N$) of the radiation beam (2a) as coherently scattered in the object to enter the line detector and be detected therein. Each of the line detectors has an elongated opening (30) for entry of the respective scattered ray bundle; a row of detector elements (27) arranged parallel with the opening; and is of the kind wherein charges or photons generated by interactions between the respective scattered ray bundle and a detection medium and traveling in a direction perpendicular to the respective scattered ray bundle, are detected by the detector elements. The line detectors and their respective detector elements are oriented to allow simultaneous recording of scatter data sufficient to form multiple one-dimensional images, each being composed of radiation as scattered in the object in a respective angle.

(Fig. 1)




46 8 6612119.

Int. t. Patent- och reg.verket

2003 -11- 0 3

Huvudfaxen Kasse

1/4

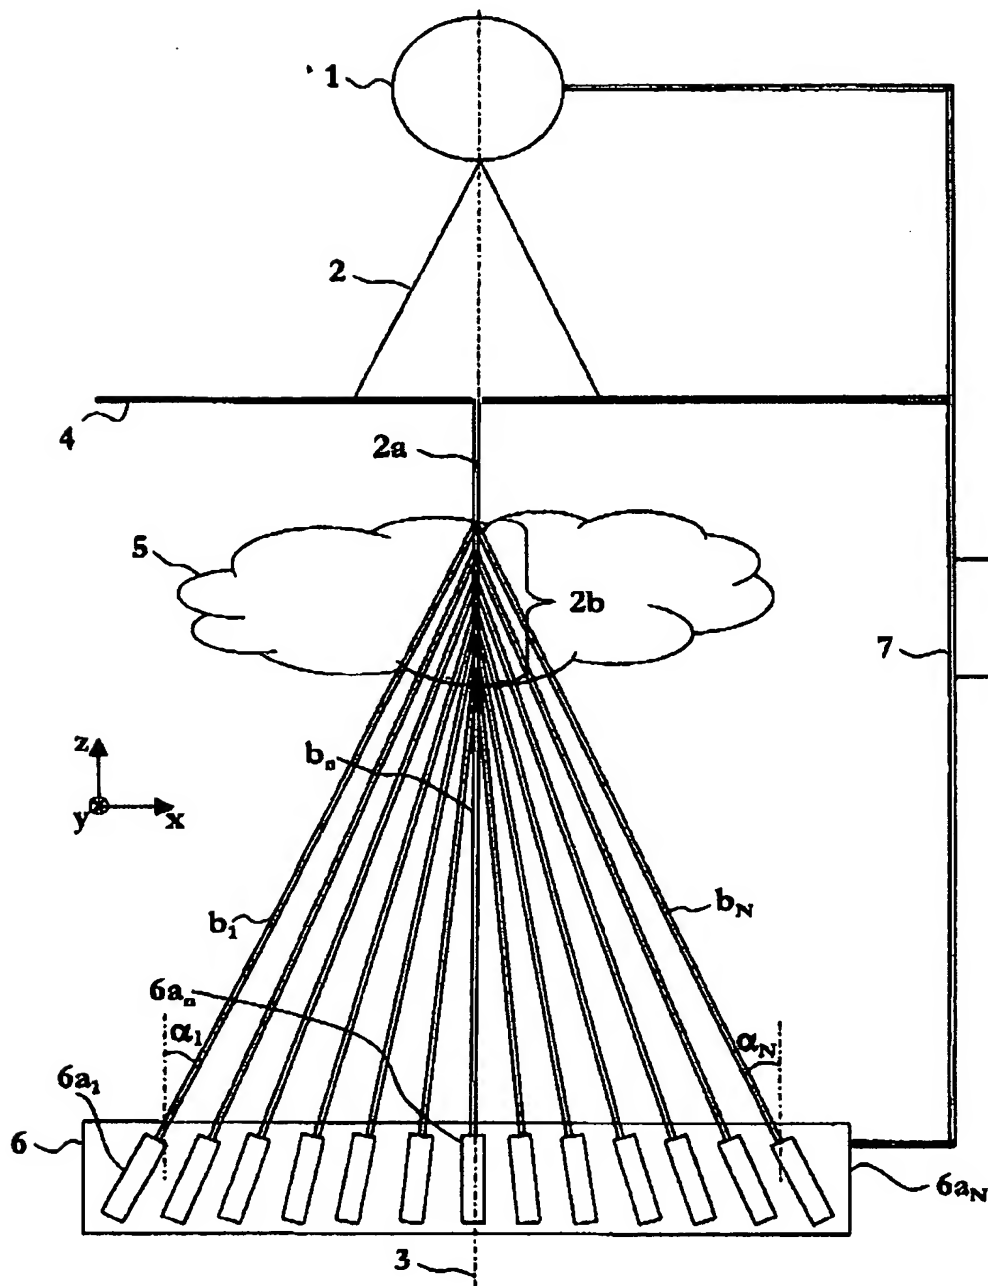**Fig. 1**

Ink. i Patent- och reg.verket

2003 -11- 0 3

Huvudfaxen Kassa

2/4

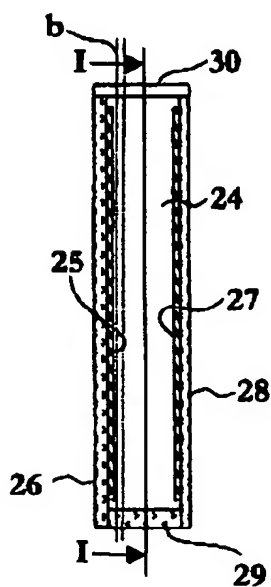


Fig. 2a

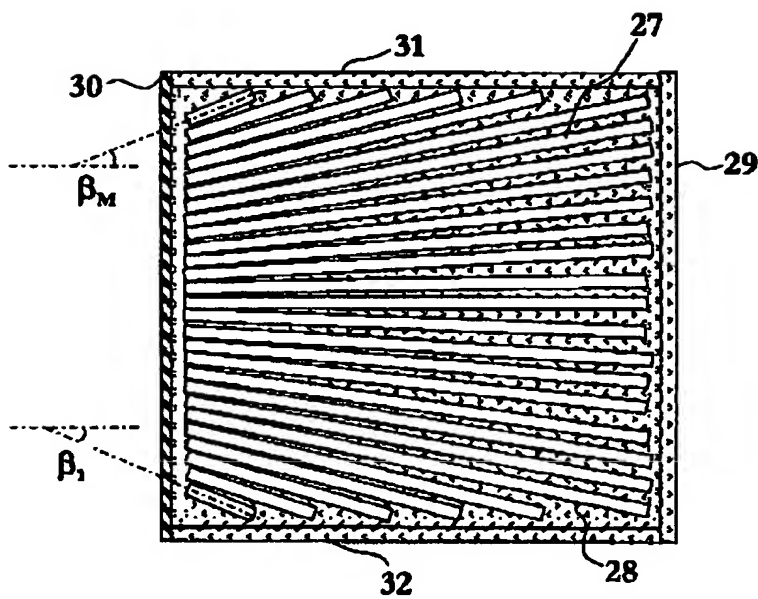


Fig. 2b

3/4

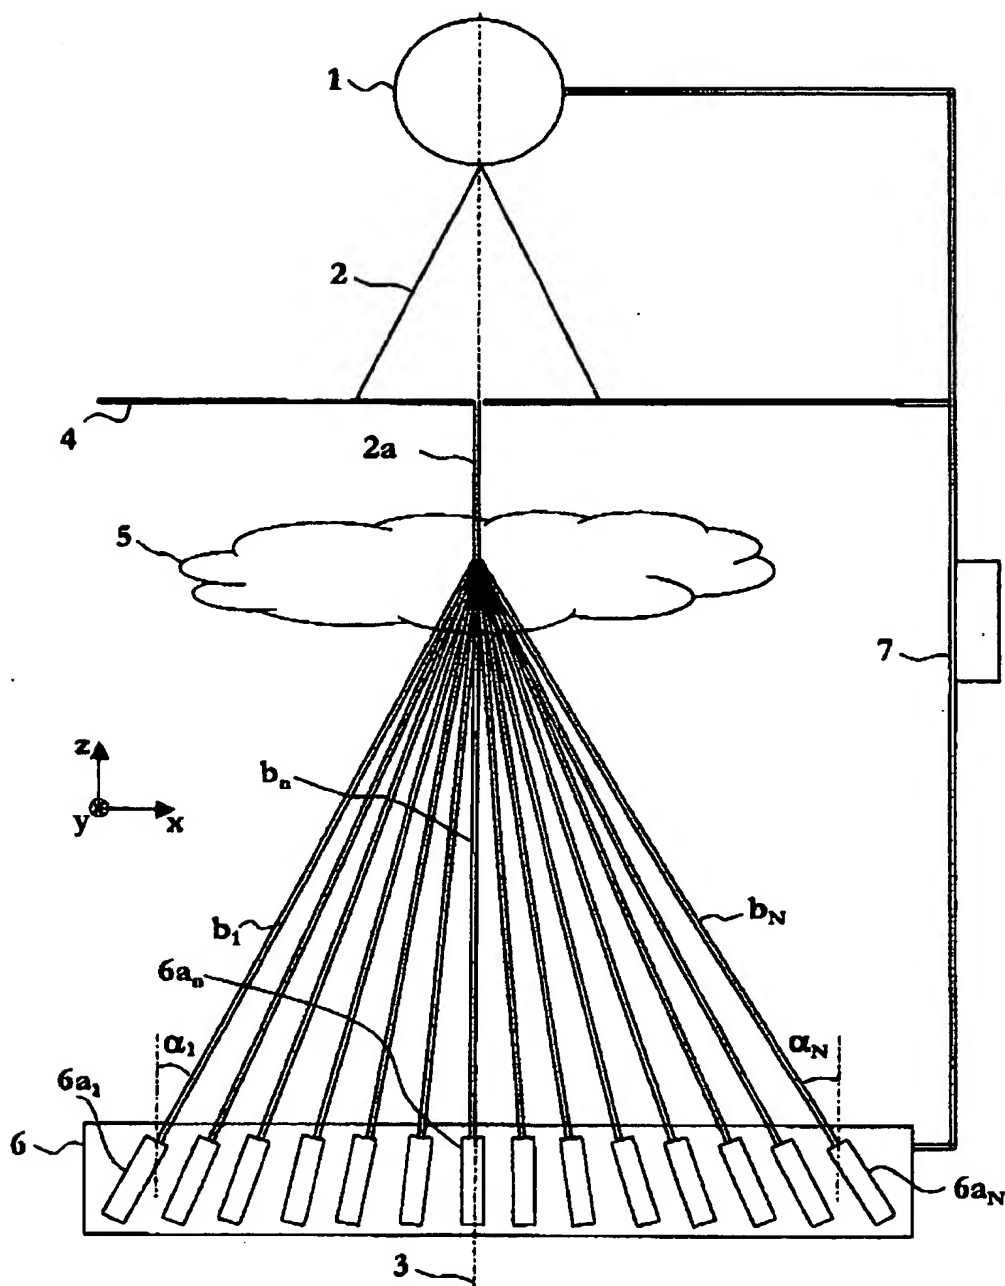


Fig. 3a

